



LSRFortessa H0081 Standard Configuration

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	7/2/2014 12:53:57 PM
Window Extension:	10.00		


Blue Laser (488nm) FSC

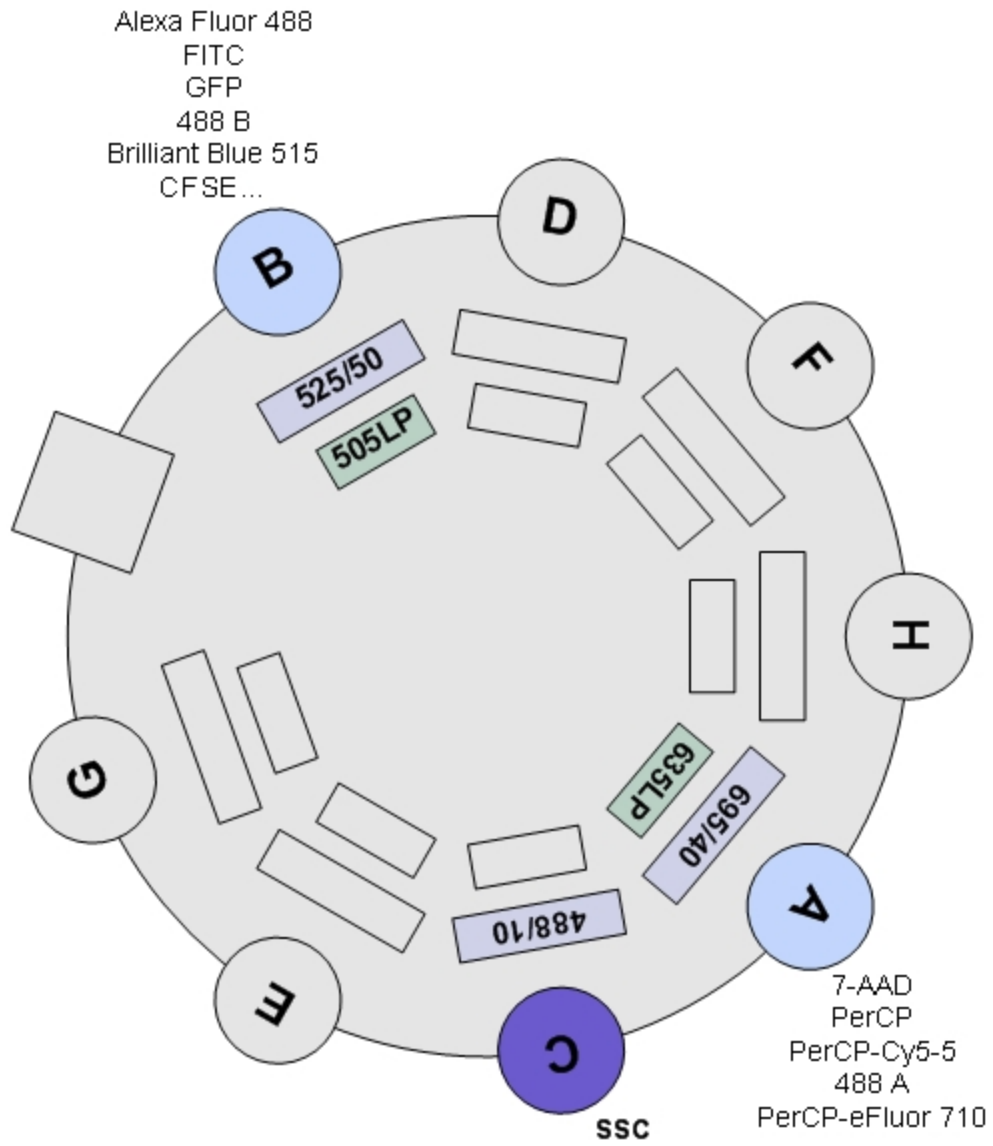


**Red Laser
(640nm)**

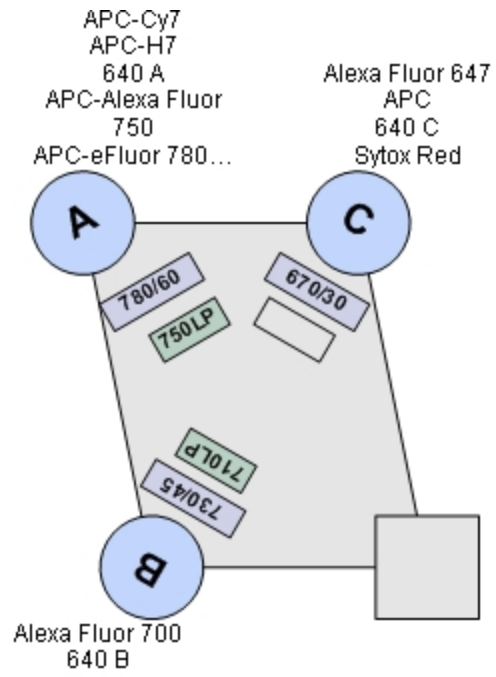


**Violet Laser
(405nm)**

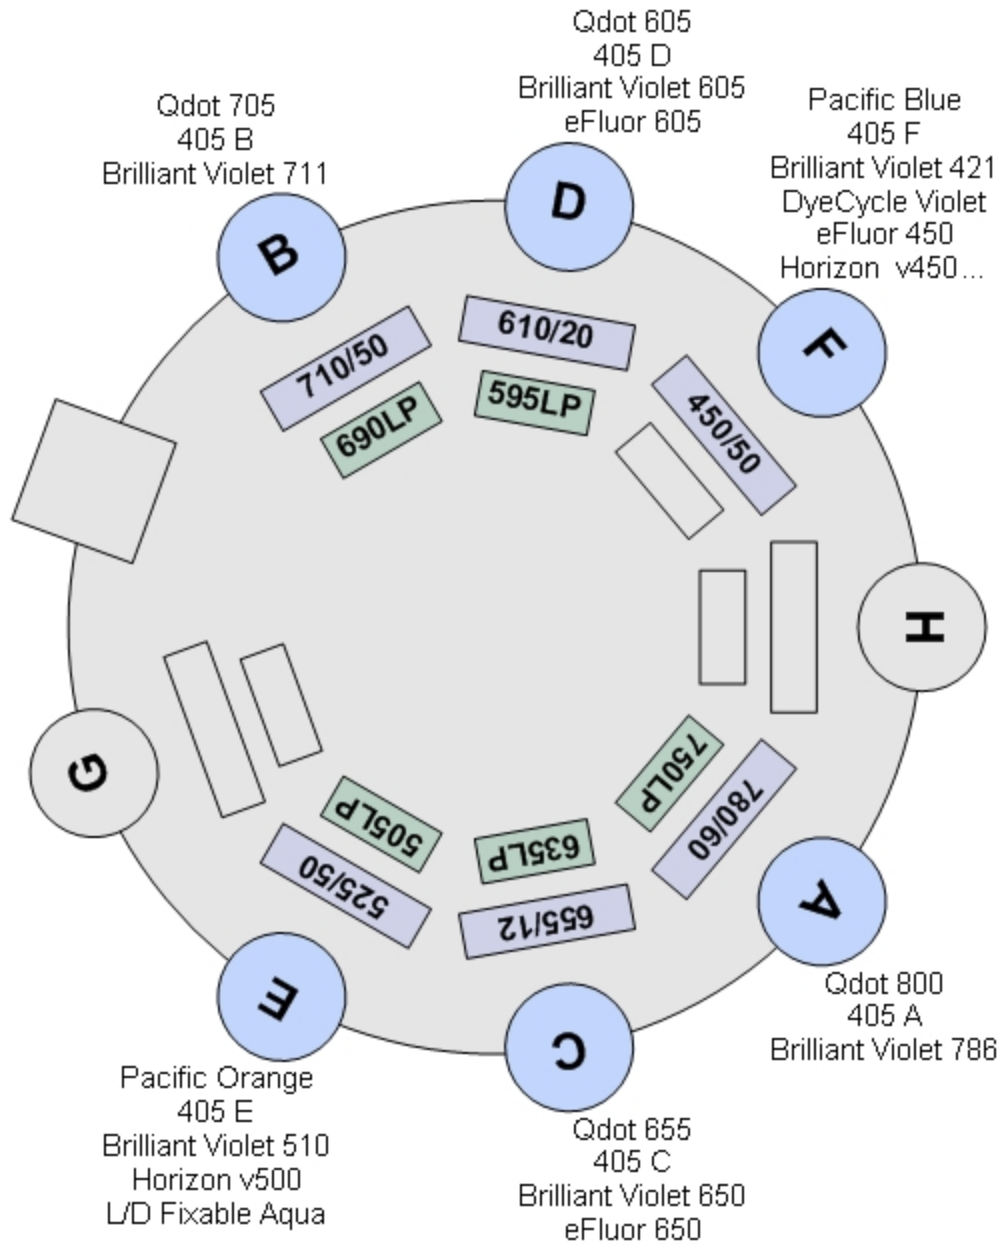

**YelGreen Laser
(561nm)**

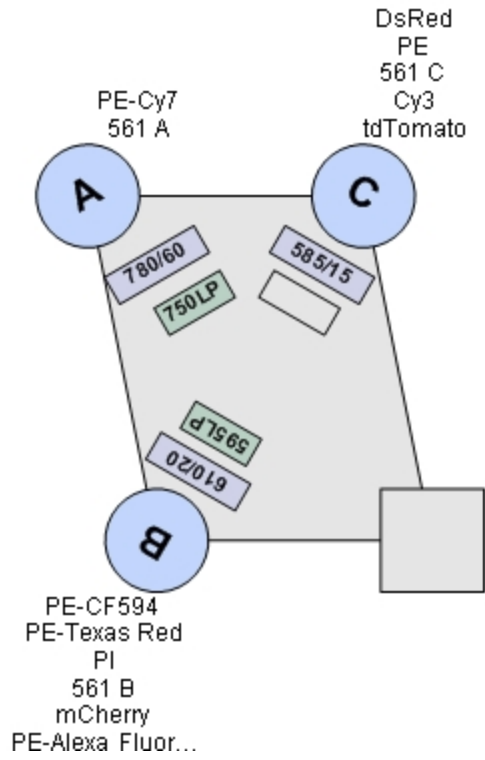

**UV Laser
(355nm)**

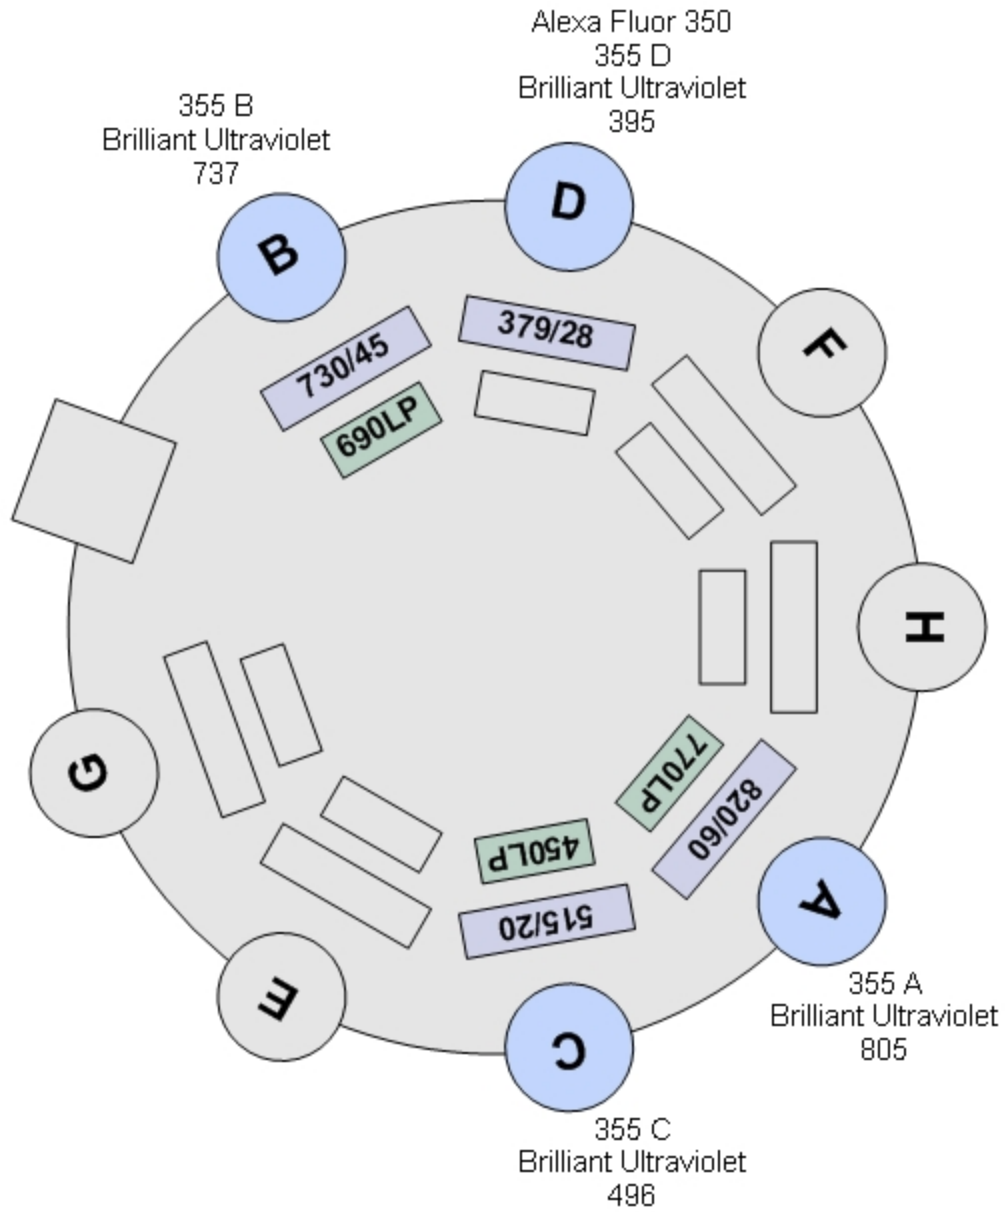

Comments: