



LSRII H4710 Standard Configuration

| | | | |
|-------------------|--------|--------------|---------------------|
| Cytometer: | LSRII | User: | BDSERVICE |
| Cytometer Name: | LSRII | Institution: | N/A |
| Serial Number: | 1 | Software: | BD FACSDiva 8.0 |
| Input Device: | Manual | Date: | 3/3/2015 1:06:53 PM |
| Window Extension: | 10.00 | | |


Blue Laser
(488nm)
FSC

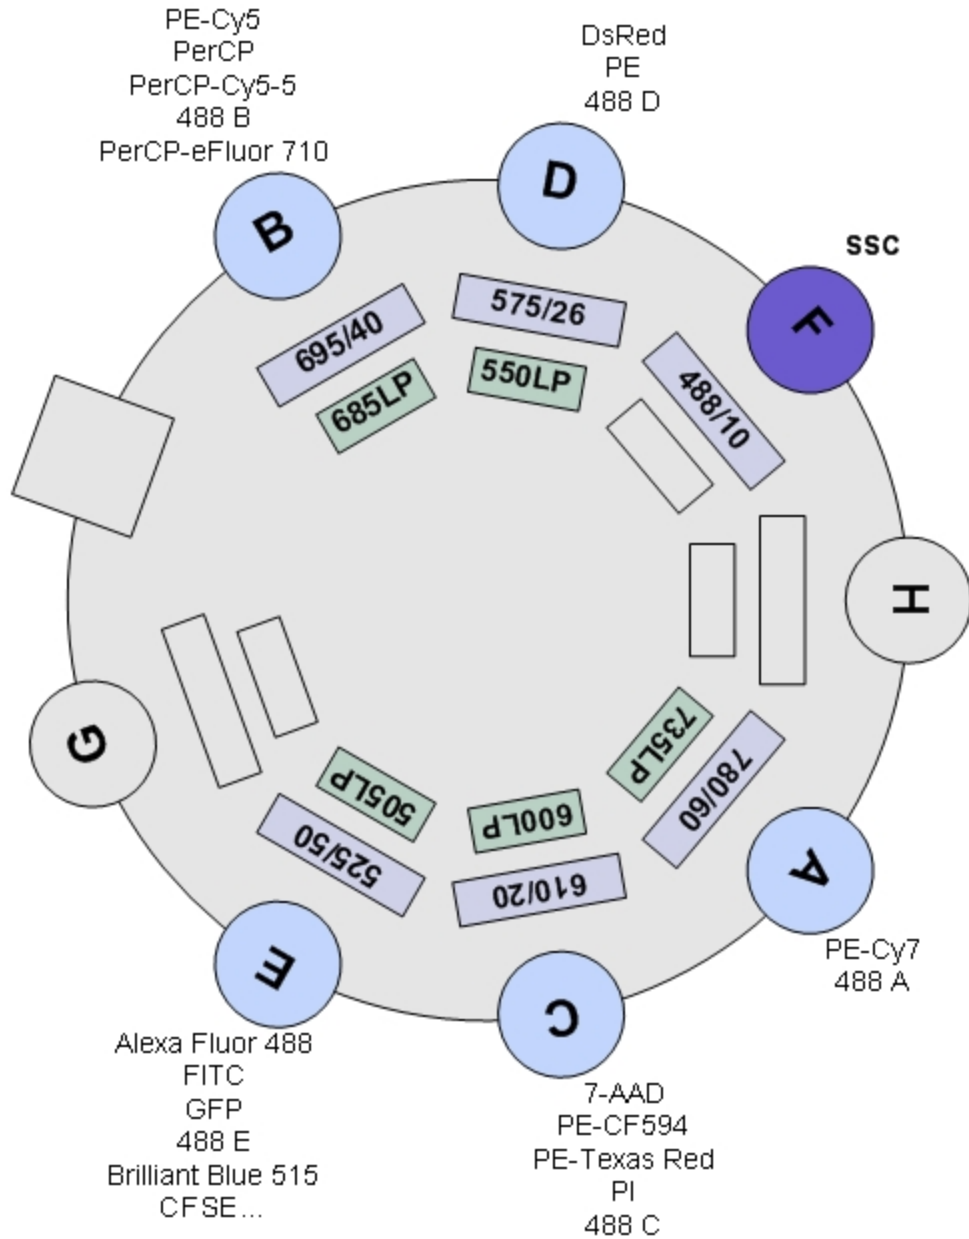


355 UV Laser
(355nm)

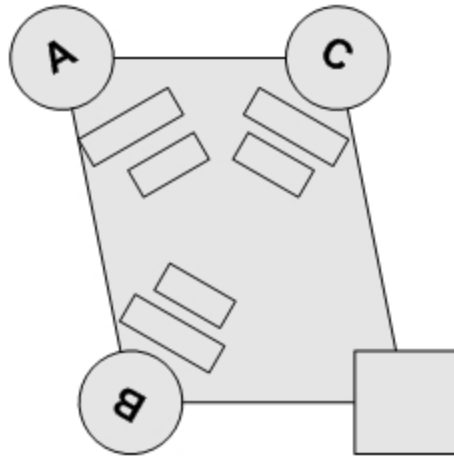

Red Laser
(633nm)

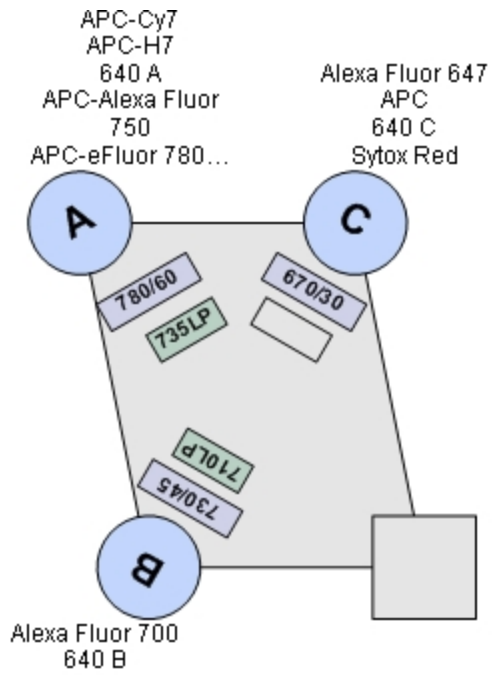

Violet Laser
(405nm)

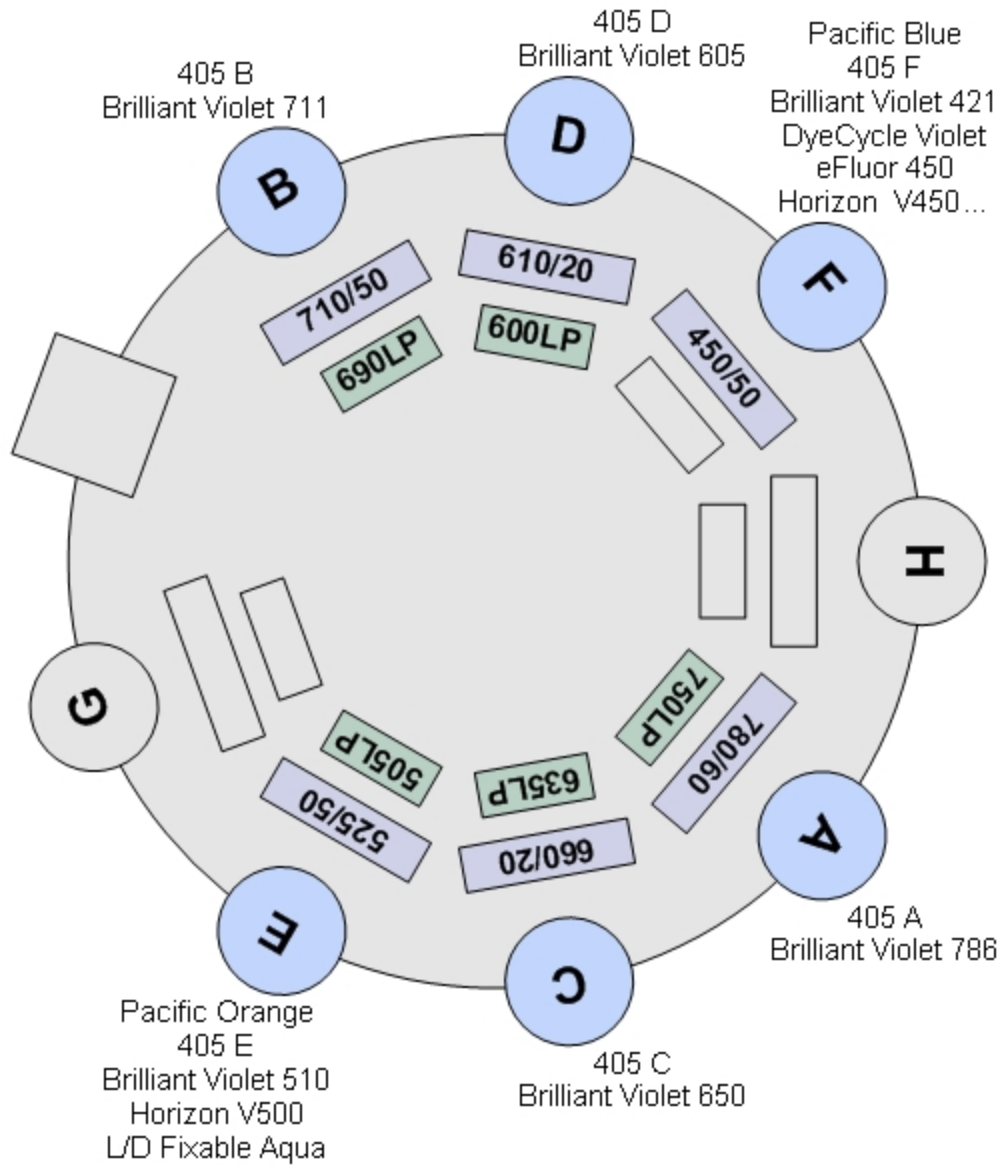

Comments: