



# H0081\_ X20 Standard Configuration 093014


Cytometer:	LSRFortessa	User:	corestaff
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	10/27/2014 10:53:31 AM
Window Extension:	10.00		

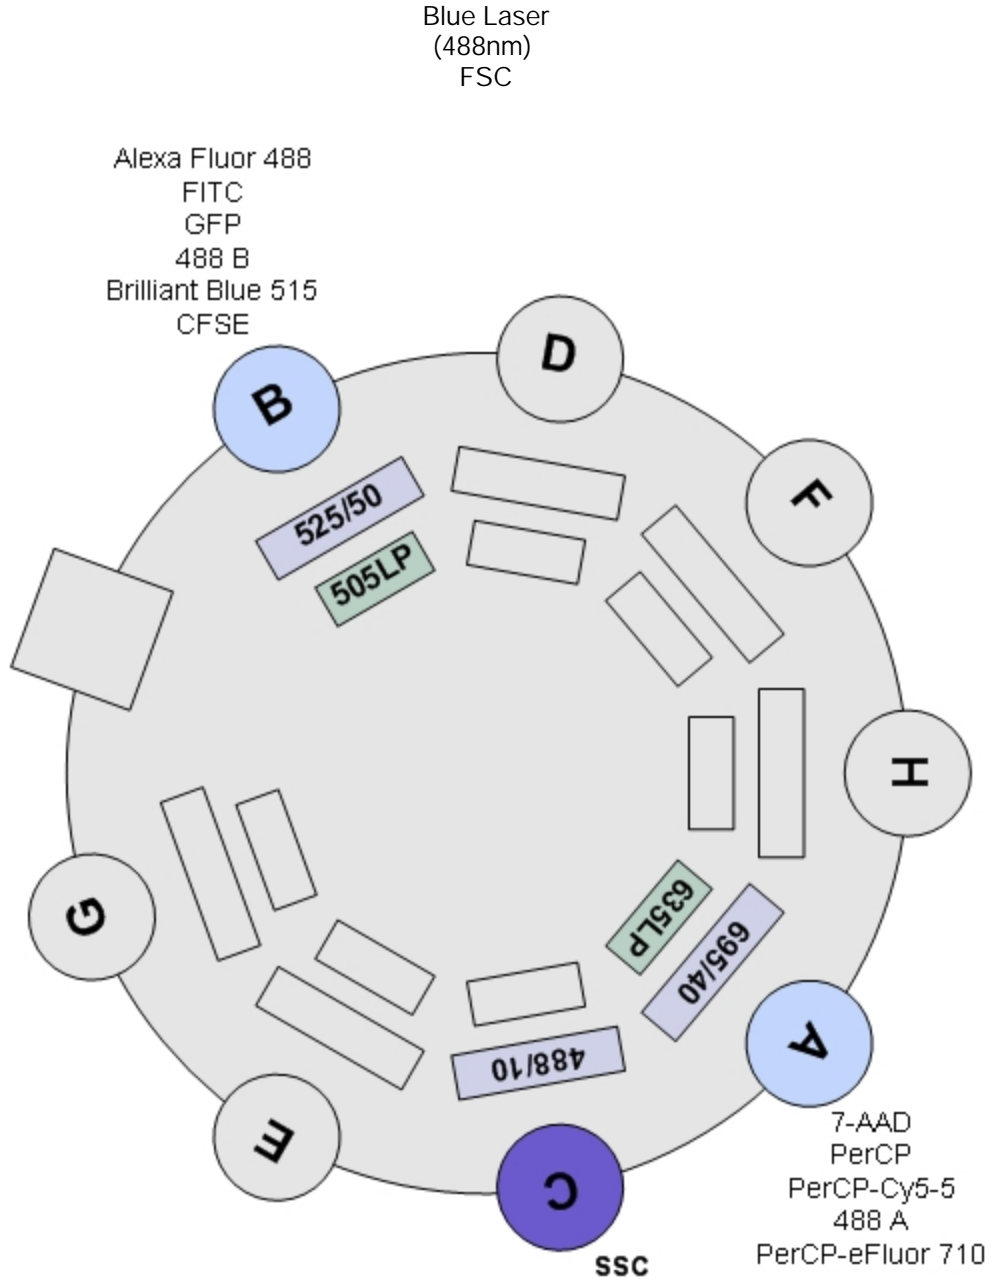

Violet Laser  
(405nm)

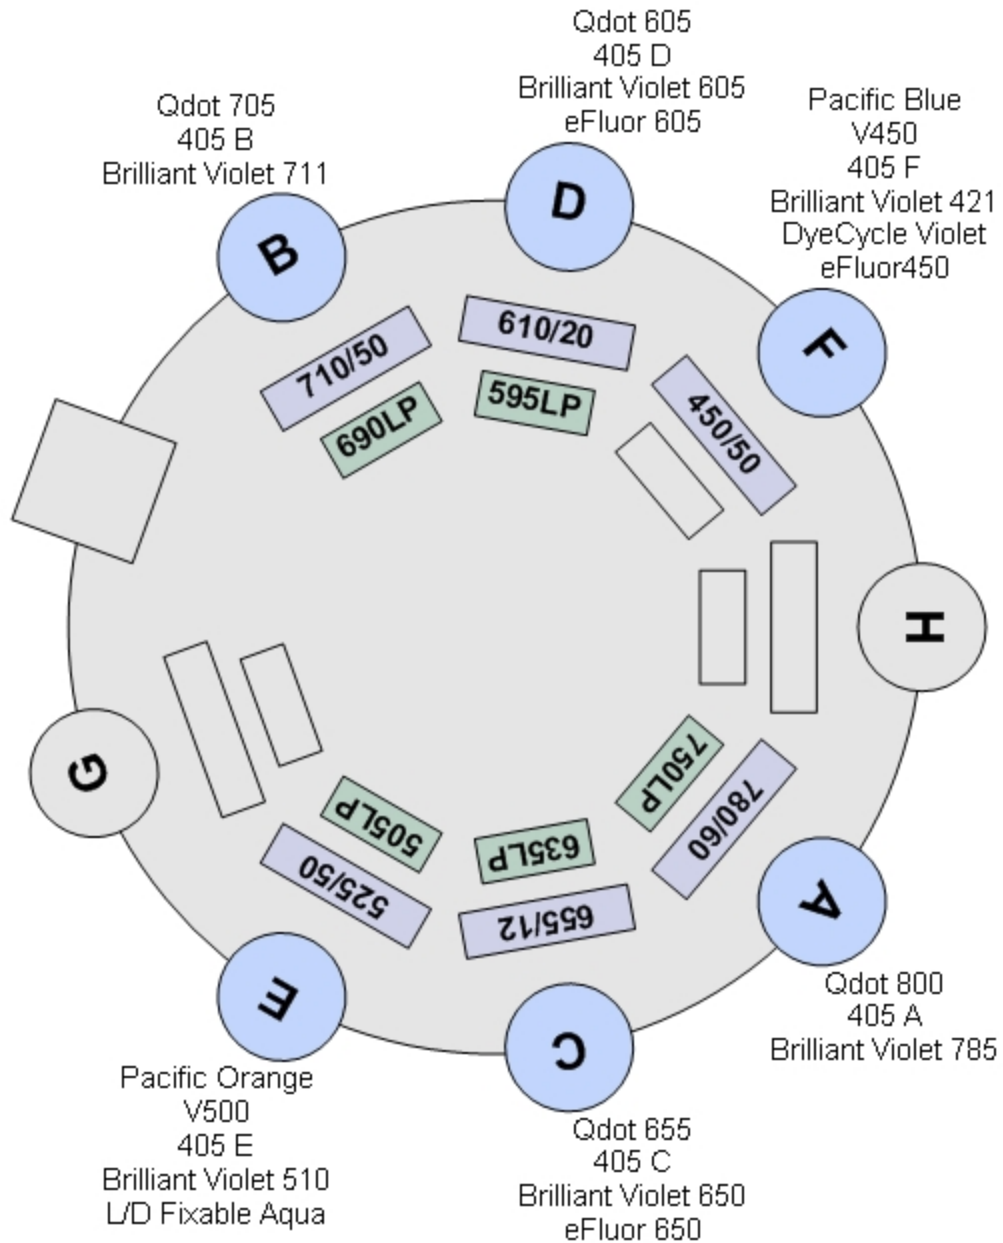


Red Laser  
(640nm)

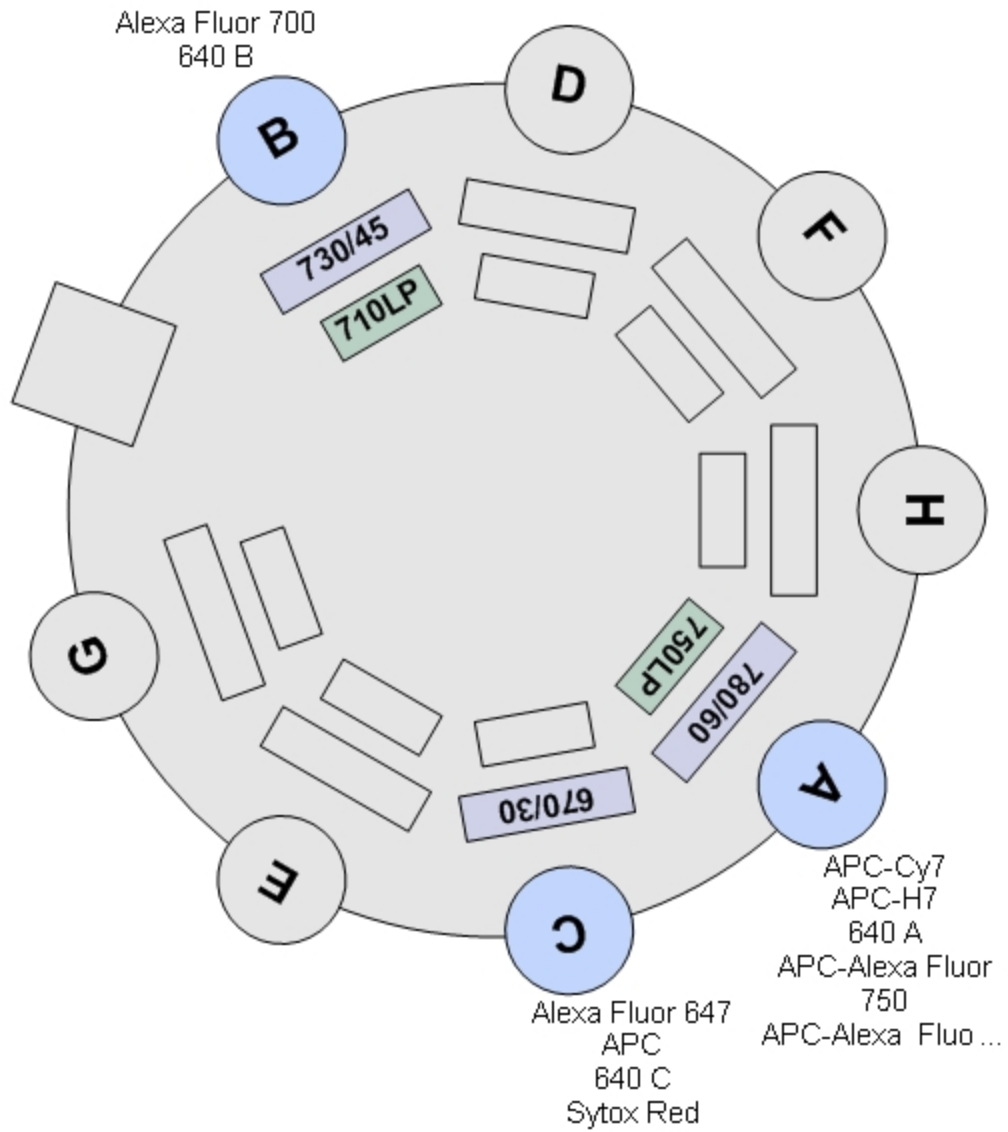


Yellow Green Laser  
(561nm)

PE-CF594  
PE-Texas Red  
561 B  
mCherry  
PE-Alexa Fluor  
610

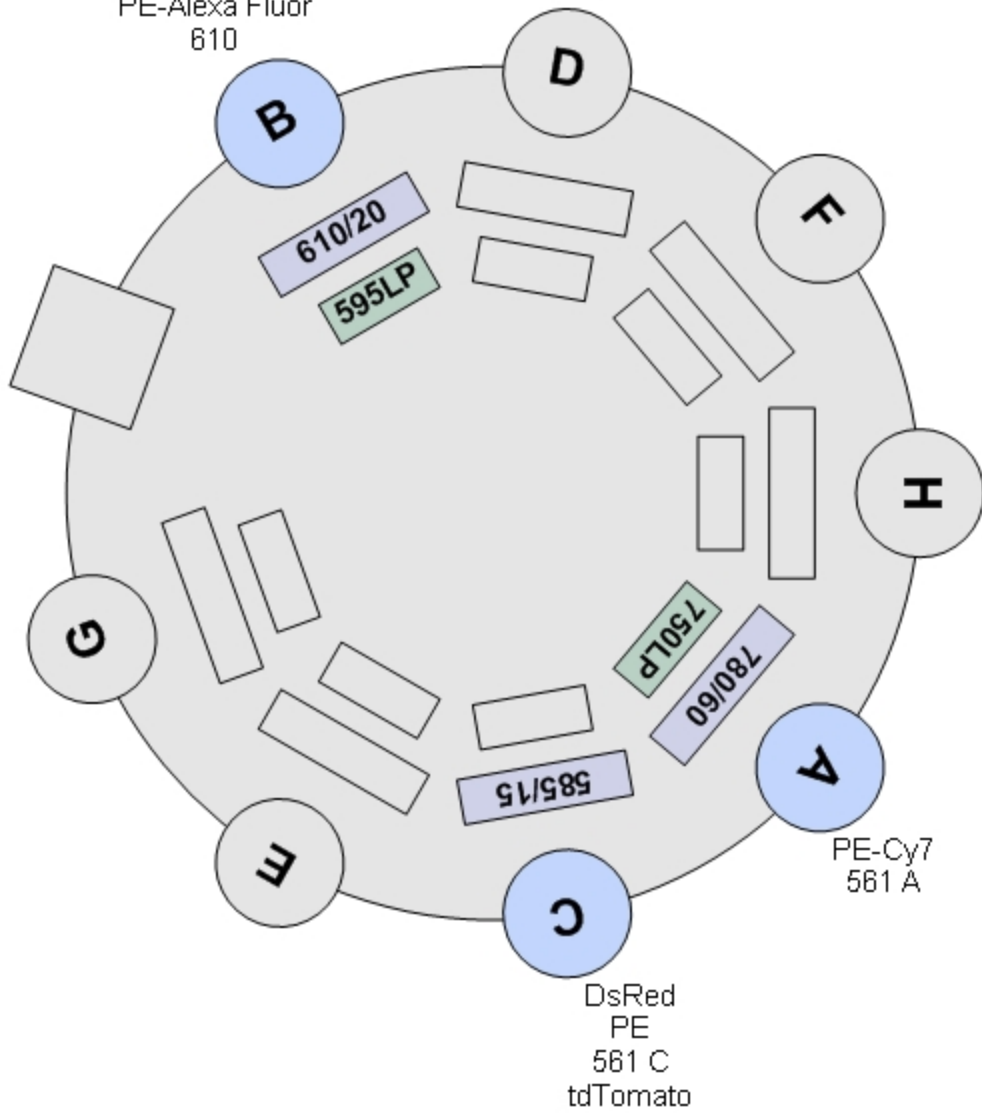

UV Laser  
(355nm)

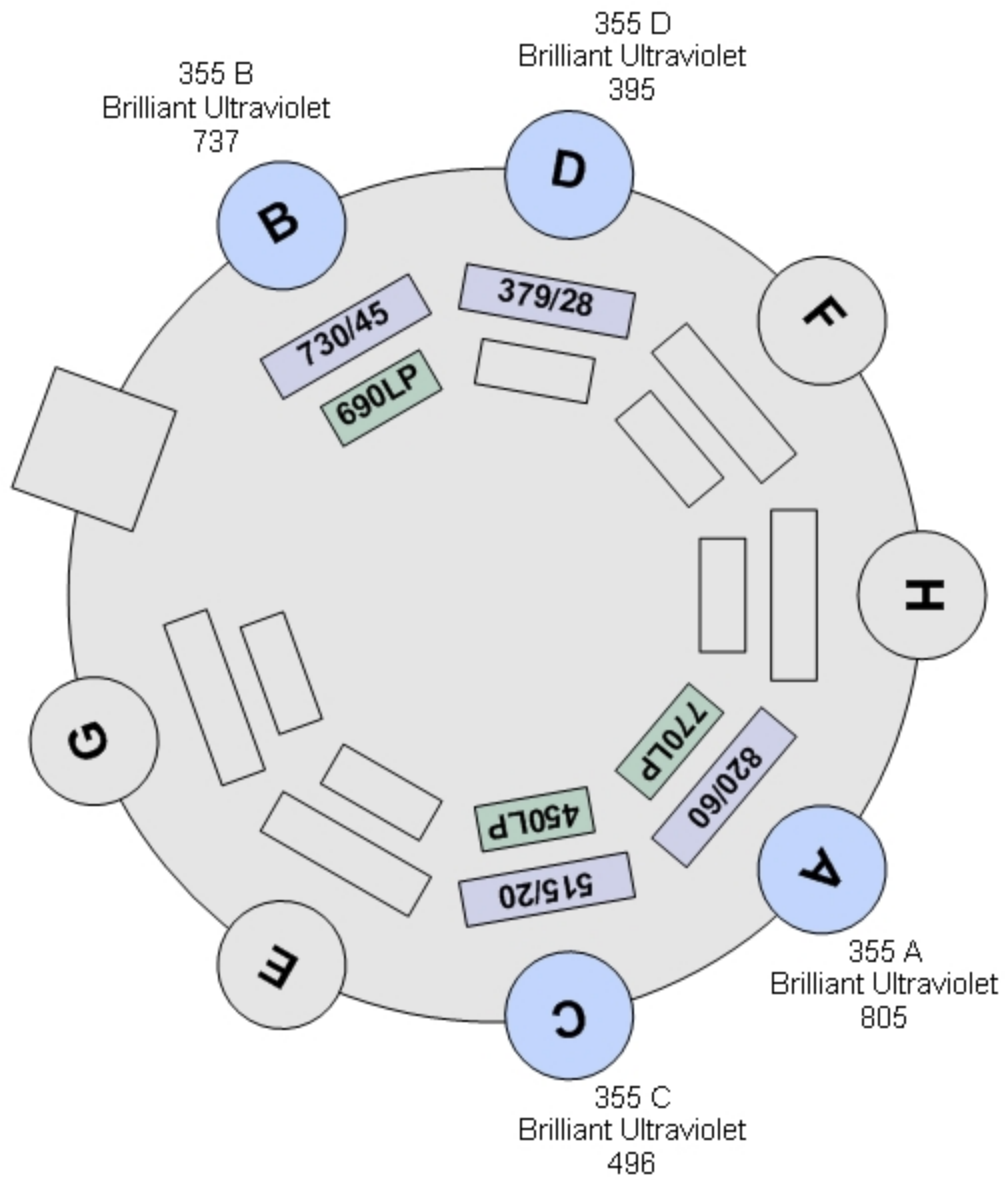

Comments: